



# MULTI WIRE MYOGRAPH SYSTEM

## MODEL 620M



---

## TRADEMARKS

Pentium is a registered trademark of the Intel Corporation. Windows, Windows 95, Windows 98, Windows ME, Windows NT, Windows 2000, Windows XP, Windows Vista, and Windows 7 are registered trademarks of Microsoft Corporation. All other trademarks are the properties of their respective owners.

DMT reserves the right to alter specifications as required.

This document was, as far as possible, accurate at the time of printing.

Changes may have been made to the software and hardware it describes since then.

New information may be supplied separately.

This documentation is provided with the DMT Multi Wire Myograph System – Model 620M

All rights reserved. No part of this manual may be reproduced or transmitted in any form or by any means without the written permission of Danish Myo Technology A/S.

Every attempt is made to ensure accurate information, misprints, construction- and specification changes, can occur.

Danish Myo Technology A/S reserves the right to alter/change content as required and without any notice.

Copyright © Danish Myo Technology A/S

# CONTENTS

Trademarks .....	3
Introduction .....	5
Safety .....	6
EMC/EMI .....	7
Approvals .....	7
Certificate of Conformity .....	8
About this manual .....	9
Unpacking the myograph system .....	10
Chapter 1 - System overview .....	11
1.1 Interface Front Panel .....	11
1.2 Interface Rear Panel .....	11
1.3 Multi wire myograph unit .....	12
Chapter 2 - Setting up .....	13
2.1 The Complete Myograph 620M System .....	13
2.2 Setting up step-by-step .....	13
2.3 The first force transducer calibration .....	14
Chapter 3 - The Interface Menus .....	15
Chapter 4 - The Multi Wire Myograph Unit .....	23
4.1 Changing and adjusting the mounting supports .....	23
4.2 Calibration of the force transducer .....	26
4.3 Checking the force transducer .....	28
4.4 Force Transducer Replacement .....	29
4.5 Myograph Maintenance .....	30
Appendix 1 - System specifications .....	32
Notes .....	33

## INTRODUCTION

Until the mid-1970s most of the information about the mechanical, morphological and pharmacological properties of vascular smooth muscle were only obtainable from studies on relatively large vessels. At that time rat-tail arteries were the smallest vessels to be investigated in detail due to limitations in the available *in vitro* techniques. For example, studies measuring the contraction force were routinely performed with only one of the mounting wires secured. Furthermore, relatively large wires (100-200  $\mu\text{m}$ ) were used, which precluded the use of small vessels. In addition, the vessel segment had to be directly manipulated with dissecting instruments, causing mechanical trauma. Investigations of smaller vessels, therefore, were limited to *in vivo* perfusion experiments and histological examination.

In 1976 Professor M. J. Mulvany and Professor W. Halpern described, for the first time, a new technique that made it possible to investigate highly isometric responses from vessels with internal diameters as small as 100  $\mu\text{m}$ . The mounting procedure was refined in 2 ways: 1) both ends of each mounting wire were secured under tension without any direct manipulation of the vessel, and 2) segments of small vessels could not be atraumatically mounted as ring preparations in a myograph for recording of highly isometric force measurements.

During the late 1970s, some improvements were made to the myograph, and in 1981, a new dual myograph that allowed simultaneous testing of two vessels was introduced. In parallel, the technique became widely acknowledged, resulting in a growing interest in the myograph systems. In 1986, the growing demand resulted in the foundation of the private company, J. P. Trading, with the purpose of making the myograph systems commercially available worldwide. At the same time, J. P. Trading initiated a comprehensive improvement programme for the existing myograph systems as well as a development programme of new myograph systems in close co-operation with Professor M. J. Mulvany and The University of Aarhus.

During the late 1980s and through the 1990s, several improvements were applied to the myograph systems, such as a new mechanical design, a more robust transducer, and a new electronic system. New systems also were introduced, such as the automatic dual myograph 510A, the multi myograph 610M and the confocal myograph 120CW. In 2000, J. P. Trading changed its company structure and became known as DMT - Danish Myo Technology A/S.

Today, DMT is one of the world's leading designers and manufacturers of wire myographs, pressure myographs, culture myographs and organ/tissue baths. Driven by our global customer base, our singular goal is to develop and manufacture first-class research equipment within the fields of physiology and pharmacology.

## SAFETY

The 620M Multi Wire Myograph System has been designed for use only in teaching and research applications. It is not intended for clinical or critical life-care use and should never be used for these purposes, or for the prevention, diagnosis, curing, treatment, or alleviation of disease, injury, or handicap.

- Do not open the unit; the internal electronics pose a risk of electric shock.
- Do not use this apparatus near water.
- To reduce the risk of fire or electric shock, do not expose this apparatus to rain or moisture. Objects filled with liquids should not be placed on the apparatus.
- Do not block any ventilation openings. Install in accordance with the manufacturer's instructions.
- Do not install near any heat sources such as radiators, heat registers, stoves, or other equipment or devices that produce heat.
- Only use attachments and accessories specified by the manufacturer.
- Unplug this apparatus during lightning storms or when unused for long periods of time.
- Be advised that different operating voltages require the use of different types of line cord and attachment plugs. Check the voltage in your area and use the correct type. See the table below:

Voltage	Line plug according to standard
110-125 V	UL81 and CSA C22.2 No. 42
220-230 V	CEE 7 page VII, SR section 107-2-D1/IEC 83, page C4
240 V	BS 1363 of 1984. Specification for 13A fused plugs and switched and unswitched socket outlets.

Protect the power cord from being walked on or pinched, particularly at power outlets and the point where they connect to the apparatus.

Refer all servicing to qualified service personnel. Servicing is required when the apparatus has been damaged in any way; such as, the power-supply cord or plug is damaged, liquid has spilled onto or objects have fallen into the apparatus, the apparatus has been exposed to rain or moisture, does not operate normally, or has been dropped.

## EMC/EMI

This equipment has been tested and complies with the limits for a Class B Digital device, pursuant to part 15 of the FCC rules. These limits are designed to provide reasonable protection against harmful interference in residential installations. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception (which can be determined by monitoring the interference while turning the equipment off and on), the user is encouraged to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different to that which the receiver is connected to.
- Consult the dealer or an experienced radio/TV technician for help.

## APPROVALS

Complies with the EMC standards:  
EMC 89/336/EEC: EN 61326-2-6:2005  
EN 61000-3-2

Certified with the safety standards:  
Directive 2006/95/EC: EN 61010-1:2001  
EN 61010-1/Corr.1:2003  
EN 61010-1/Corr.1:2003  
EN 61010-2/101:2003

## CERTIFICATE OF CONFORMITY

---

DMT A/S, Skejbyparken 152, 8200 Aarhus N., Denmark,  
hereby declares its responsibility that the following product:

*Multi Wire Myograph System - Model 620M*

is covered by this certificate and marked with CE-label conforms  
with the following standards:

EN 61010-1:2001  
EN 61010-1/Corr.1:2003  
EN 61010-1/Corr.1:2003

Safety requirements for electrical equipment for measurement, control, and laboratory use –  
Part 1: General requirements.

EN 61010-2-101:2003

Safety requirements for electrical equipment for measurement, control and laboratory use – Part 2 – 101: Particular requirements for in vitro diagnostic (IVD) medical equipment.

EN 61326-2-6:2005

Electrical equipment for measurement, control and laboratory use –  
EMC  
Requirements – Part 2-6: Particular requirements In vitro diagnostic (IVD) medical equipment.

With reference to regulations in the following directives: 2006/95/EC,  
89/336/EEC.



## ABOUT THIS MANUAL

This manual contains a complete list of procedures that describe how to install, maintain and using the Multi Wire Myograph System – Model 620M.

Chapter 1 provides an overview of the construction and basic features of the Interface and the Multi Wire Myograph Unit.

Chapter 2 describes step-by-step instructions to set up a complete 620M Wire Myograph System, including accessories.

Chapter 3 is a complete manual to the 620M Interface. This chapter describes, in detail, how to navigate the menus and how to use the special features of the 620M Myograph System.

Chapter 4 contains procedures describing general and daily maintenance of the myograph unit; e.g. adjustment of supports, weight calibration of the force transducer and cleaning instructions.

Appendix contain additional information such as system specifications.

## UNPACKING THE MYOGRAPH SYSTEM

Take a few minutes to carefully inspect your new Multi Wire Myographs System - 620M for damage which may have occurred during handling and shipping. If you suspect any kind of damage, please contact DMT immediately and the matter will be pursued soon as possible. If the packing material appears damaged, please retain it until a possible claim has been settled.

We recommend that you store the packing material for any possible future transport of the Wire Myograph System. In case of transport and the original packing material is unavailable, please contact DMT Sales Department for advice and packing instructions.

After unpacking your new Multi Wire Myograph System, please use the following list to check that the system is complete:

- 1 interface unit
- 4 chamber units with mounted stainless steel jaws
- 4 set mounting support pins (200µm)
- 4 chamber covers
- 1 external temperature probe
- 1 power cord\*
- 1 calibration kit (including “bridge”, “balance” and 2 gram weight)
- 4 plastic funnels
- 1 roll of 40 µm stainless steel wire
- 1 tube of high vacuum grease
- 1 tube of grease for linear slides
- 5 spare screws for mounting of jaws
- 3 Allen keys
- 1 small screwdriver
- 1 CD with user manuals for Wire Myograph Systems
- 1 CD with the manual “Procedures for investigation of small vessels using small vessel myograph”, by Professor M. J. Mulvany, Department of Pharmacology, Aarhus University, Denmark and the video “Dissection and mounting of small vessels in wire myographs”

\* *The shape of the AC plug varies by country; be sure that the plug fits the outlets for your location.*

# CHAPTER 1 - SYSTEM OVERVIEW

## 1.1 Interface Front Panel

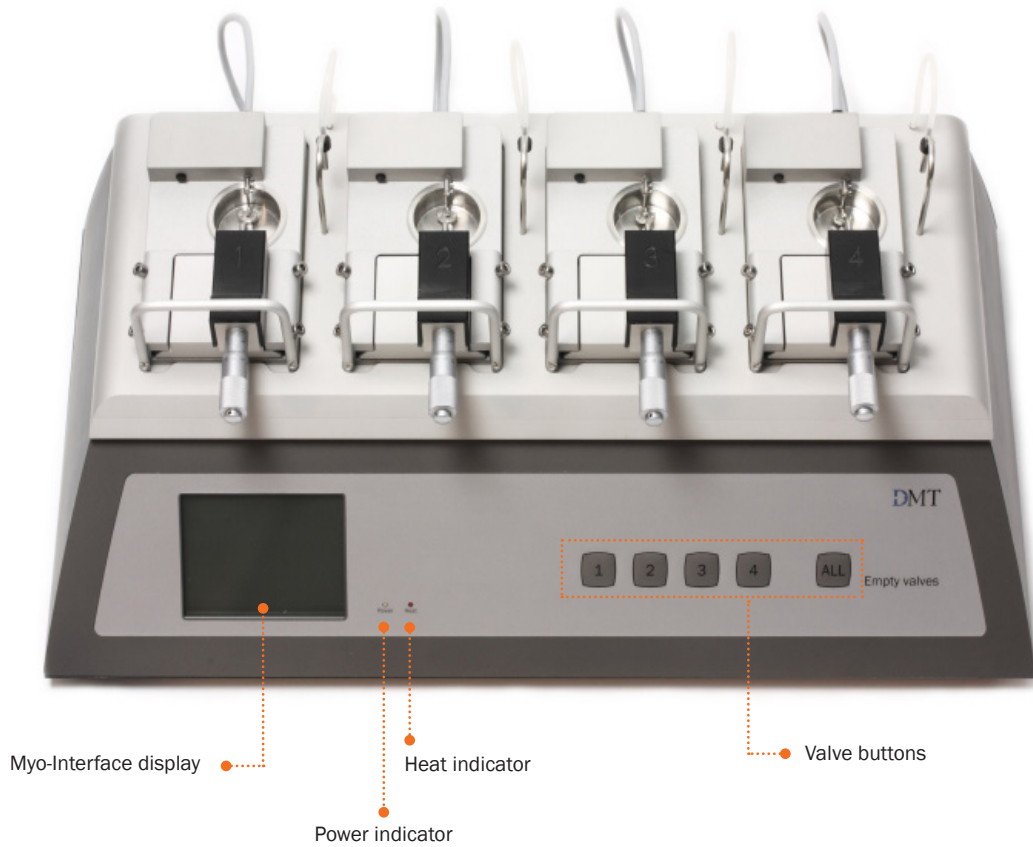


Figure 1.1 Interface Front Panel

## 1.2 Interface Rear Panel

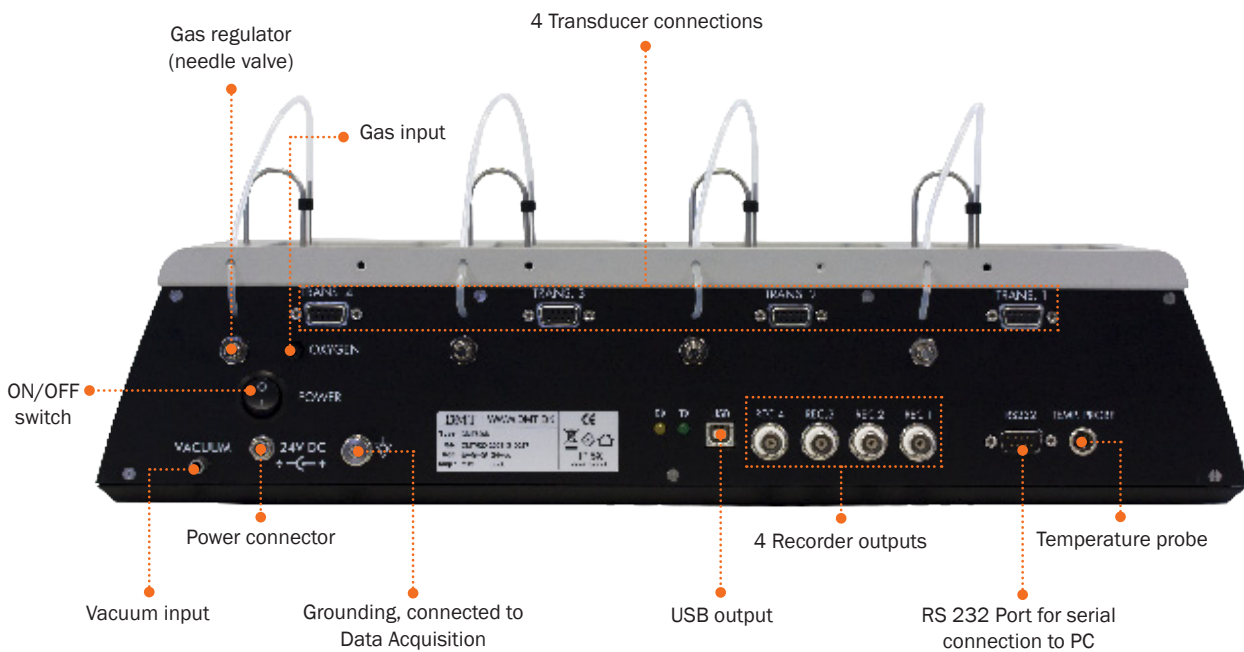


Figure 1.2 Interface Rear Panel

### 1.3 Multi wire myograph unit

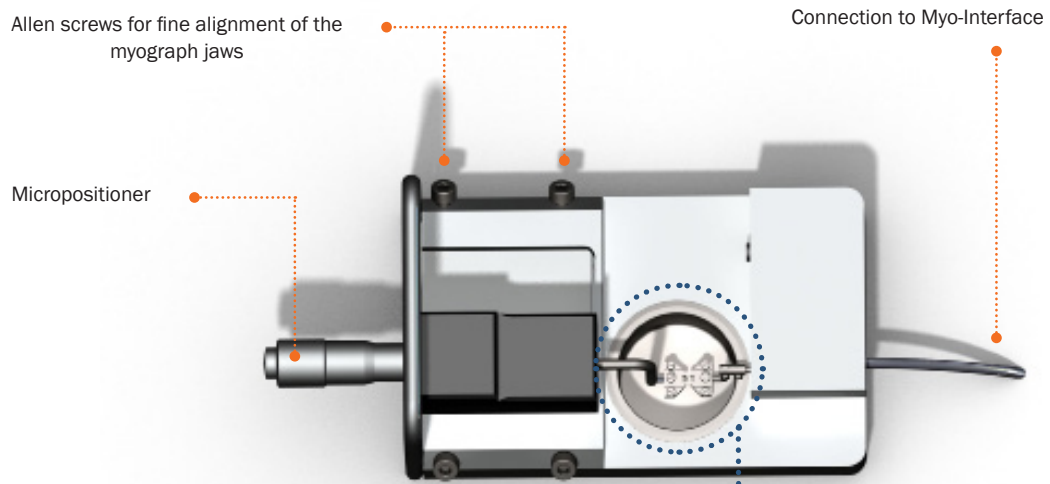


Figure 1.3 Multi Wire Myograph unit

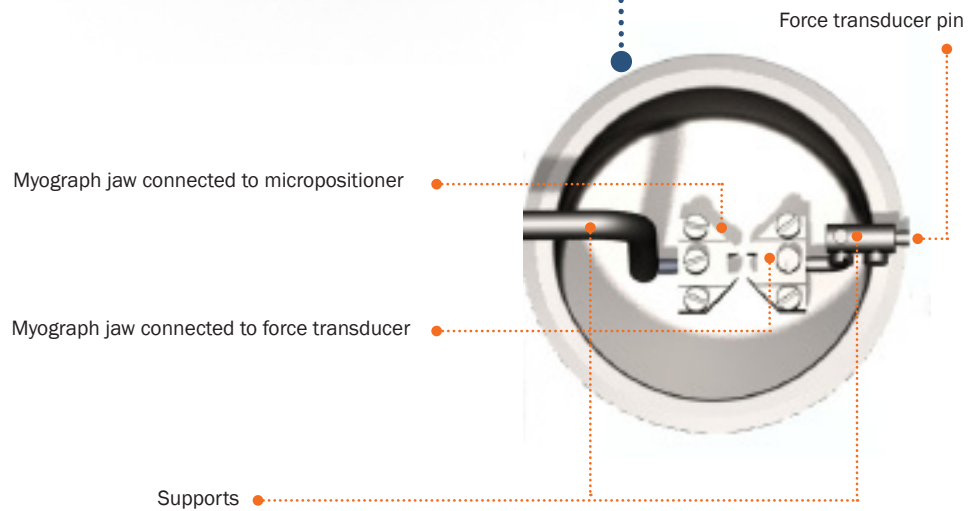


Figure 1.4 Close up of myograph jaws

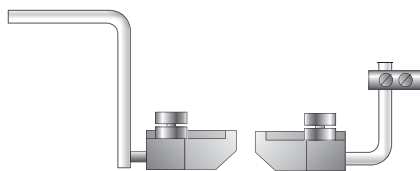


Figure 1.5 Mounting jaws for small vessels



Figure 1.6 Mounting pins for larger vessels

## CHAPTER 2 - SETTING UP

### 2.1 The Complete Myograph 620M System

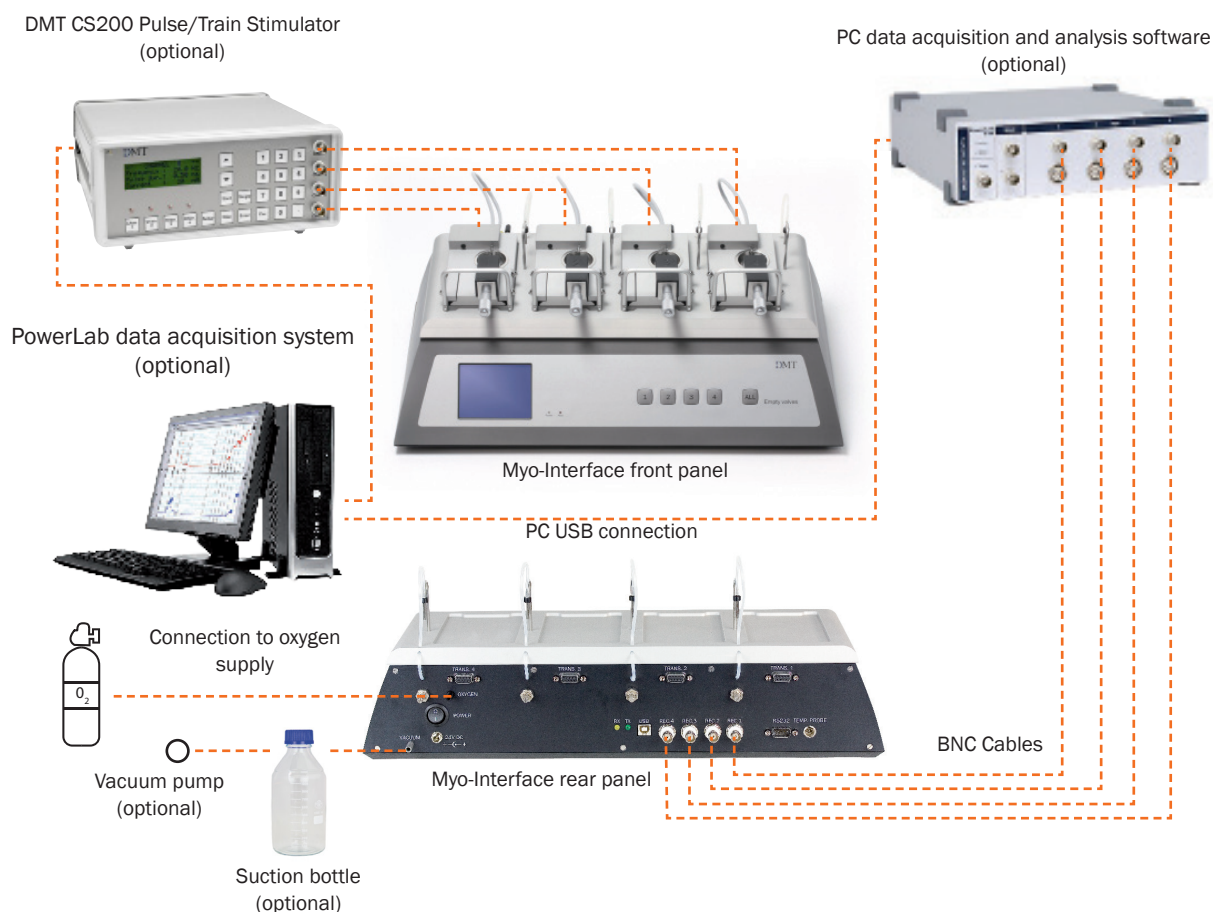


Figure 2.1 The complete Multi Wire Myograph System - Model 620M

### 2.2 Setting up step-by-step

This chapter contains a complete step-by-step description of how to set up a complete myograph 620M system as illustrated in Figure 2.1 above.

1. Interface – PC Connection:  
Data acquisition is possible either by connecting the Interface directly to a PC or through a PowerLab data acquisition and analysis system (optional).
  - I. Direct PC Connection:  
Connect the Interface to one of the COM-ports on the PC using a serial cable (cable not included).
  - II. PowerLab (Optional):  
Connect the Interface to the PowerLab unit using BNC cables. Connect Rec 1 on the Interface to Input 1 on the Power Lab, Rec 2 to Input 2 etc. Connect the PowerLab unit to one of the USB-ports on the PC using the USB cable delivered with the PowerLab system.
2. Oxygen Supply:  
Connect the gas supply (95% O<sub>2</sub>, 5% CO<sub>2</sub> or 21% O<sub>2</sub>, 5% CO<sub>2</sub>, balance N<sub>2</sub>) with tubing running from the gas supply to the gas inlet on the back of the Interface. Oxygen is supplied to the chambers by tubing attached to the stainless steel vacuum pipe. The oxygen and vacuum tubing need to be inserted into the chamber in order to aerate the heated buffer. Needle valves on the back of the interface can be adjusted to regulate the amount of bubbling that occurs. Turning the regulator clockwise increases the bubbling while turning it counter-clockwise decreases the bubbling. Each regulator has a lock device attached that can be used when the desired bubbling is achieved. See Figure 2.2 on next page.

NOTE: THE NEEDLE VALVES NEED TO BE GREASED (USING THE GREASE FOR THE LINEAR SLIDES) AND TURNED AT REGULAR INTERVALS TO PREVENT THEM FROM STICKING OR PERMANENTLY FREEZING.

### 3. Vacuum Connection:

The system has a built-in manifold with separate valves that allows each chamber to be drained individually. After connecting the vacuum source at the back of the Interface, the vacuum pipes need to be inserted into the chambers in order for this feature to work properly. The pipes are inserted into the chamber by gently pulling up on the curved part of the pipe, turning it 90° counter-clockwise and gently lowering it into the chamber. A chamber can then be emptied by pressing the corresponding numbered button. Pressing the “all” button will empty all the chambers at the same time, see Figure 2.2 below.

NOTE: WHEN DRAINING THE CHAMBERS USING THE AUTOMATIC VACUUM FUNCTION, PRESS THE APPROPRIATE BUTTON FOR AN ADDITIONAL 3-5 SECONDS AFTER THE INITIAL EMPTYING. THIS WILL HELP DRAIN RESIDUAL BUFFER AND SOLUTIONS RETAINED IN THE TUBING AND VALVES.

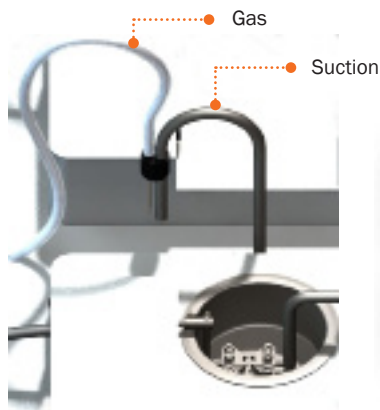


Figure 2.2 Suction connection

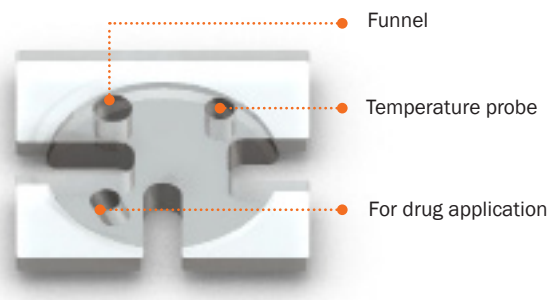


Figure 2.3 Chamber cover

### 4. Chamber Covers

The chamber covers will help maintain the temperature and other buffer conditions (gas tension, pH) fairly constant. Holes in the chamber covers serve different purposes, and they are illustrated in Figure 2.3 above. The slots allow the covers to be placed over the chamber around the support arms and gas/vacuum tubes.


## 2.3 The first force transducer calibration

Prior to the shipment of the Multi Wire Myograph 620M System, has gone through two days of continuous testing, including a final force transducer calibration. However, DMT recommends that a new force transducer calibration is performed before using the myograph system for the first time. The force transducer calibration procedure is described in detail in the *FORCE CALIBRATION* sub-menu under *SETTINGS*, as explained in Chapter 3.


# CHAPTER 3 - THE INTERFACE MENUS

Chapter 3 is a complete manual for the 620M Interface. The chapter contains a detailed description of how to navigate the touch-screen menus and how to use the special features of the 620M myograph.


Menus on the 620M interface are all accessible by a touch screen. To access a menu, simply touch the screen to access a menu. When a setting needs to be changed, the setting can be changed by pressing the "SELECT" icon on the touch screen corresponding to the desired channel to be changed.

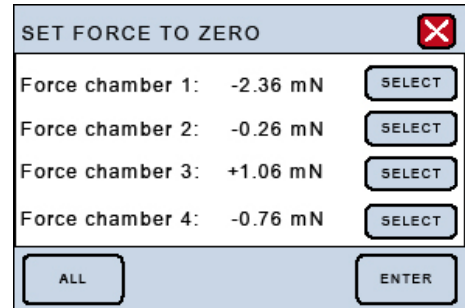

The line to be modified will turn blue, indicating that the interface is waiting for input. When "ALL" is chosen, all lines corresponding to all 4 channels will turn blue. Changing the numeric value for the chosen parameter can be done by touching the up or down arrow keys.

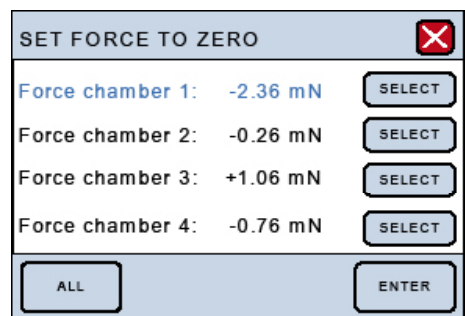


Once the desired setting has been chosen, pressing "ENTER" will lock the selection and be stored in memory. Pressing the white "X" in the red box will exit that menu and take you automatically to the Actual Force Display.

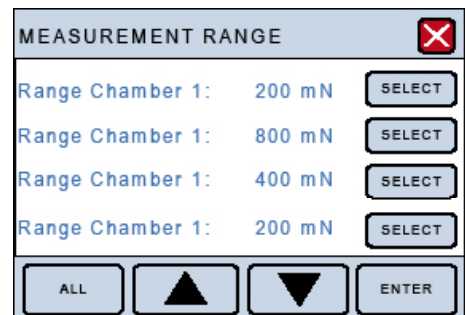


### Power-Up Screen


After turning on the 620M Interface, an "Introduction" screen appears. The system is auto-calibrating the A/D converters while this screen is displayed.

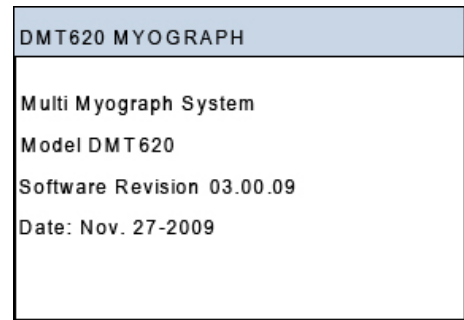


After a few seconds, the "ACTUAL FORCE" display will appear.

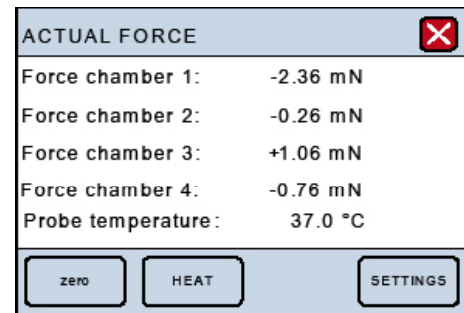

At any given time, if the force applied on any channel is out of range, the force reading for the overloaded channel will turn yellow as a warning.

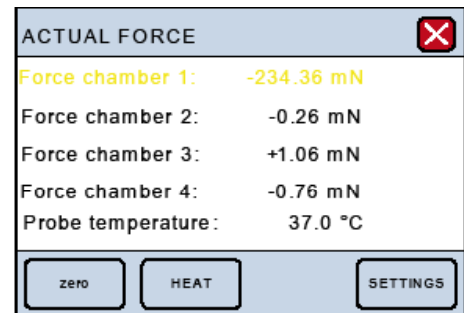

Three menus are accessible from the default "Actual Force" screen or display. These menus are: Zero, Heat, and Settings.

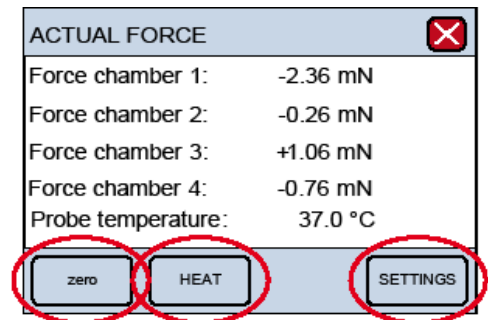



### Zero Menu:

This menu is used to zero the output of the transducers. When using a data acquisition program like LabChart by AD Instruments®, using this feature will reset the baseline of the chart traces without affecting the calibrations or physically changing any pre-load tensions placed on the mounted vessels. The channels can be changed individually by pressing “SELECT” or all at once by pressing “ALL”. Pressing “ENTER” will execute the zero function and return the user to the ACTUAL FORCE display.

SET FORCE TO ZERO		✕
Force chamber 1:	-2.36 mN	SELECT
Force chamber 2:	-0.26 mN	SELECT
Force chamber 3:	+1.06 mN	SELECT
Force chamber 4:	-0.76 mN	SELECT
ALL		ENTER

### Heat Menu:

The heating unit and temperature are controlled from this menu. To turn the heat on or change the preset temperature for the system, access the temperature control menu. Pressing the “HEAT” key will enter the menu and allow the user to change the default system temperature, as well as turn the heat on or off. Pressing “DEFAULT” will automatically reset the temperature setpoint to 37 °C. Manually change the temperature by pressing the up or down arrows.

SET CHAMBER TEMPERATURE		✕	
Temperature setpoint.	37.0 °C		
Probe temperature.	36.6 °C		
HEAT:	ON	OFF	
DEFAULT	▲	▼	ENTER

To turn the heat on, touch “ON” and the “ON” icon will turn green, indicating the heat has been turned on. The system will heat to the designated temperature setpoint.

Pressing the white “X” in the red box will send the user back to the “ACTUAL FORCE” display.

SET CHAMBER TEMPERATURE		✕	
Temperature setpoint.	37.0 °C		
Probe temperature.	36.6 °C		
HEAT:	ON	OFF	
DEFAULT	▲	▼	ENTER

### Settings Menu:

The “Settings Menu” contains several sub-menus that can be accessed to change functional aspects of the interface. These sub-menus include:

1. FORCE CALIBRATION
2. VALVE DELAY
3. FORCE REC. OUTPUT
4. MEASUREMENT RANGE
5. INTERFACE SETTINGS

SETTINGS					✕
FORCE CALIBRATION	VALVE DELAY	FORCE REC. OUTPUT	MEASUREMENT RANGE		
INTERFACE SETTINGS					

## 1. Force calibration

**NOTE: EVERYTIME A FORCE CALIBRATION IS PERFORMED THE MEASUREMENT RANGE IS SET TO DEFAULT 200 mN. SET MEASUREMENT RANGE AFTER THE FORCE CALIBRATION.**

Entering the FORCE CALIBRATION sub-menu begins the transducer calibration procedure. Begin the calibration procedure by pressing "FORCE CALIBRATION" to enter the sub-menu. The sub-menu will list all 4 chambers for calibration.

To begin the calibration, press "SELECT" for the chamber which calibration will be performed on. The text for the chamber to be calibrated will turn blue. Pressing "ENTER" will enter the 6-step procedure for calibrating the force transducer on the desired chamber.

FORCE CALIBRATION [X]

Force calibration chamber 1: [SELECT]

Force calibration chamber 2: [SELECT]

Force calibration chamber 3: [SELECT]

Force calibration chamber 4: [SELECT]

[ENTER]

FORCE CALIBRATION [X]

Force calibration chamber 1: [SELECT]

Force calibration chamber 2: [SELECT]

Force calibration chamber 3: [SELECT]

Force calibration chamber 4: [SELECT]

[ENTER]

The calibration procedure is listed in 6 individual steps and needs to be performed for each channel or transducer when calibrating the system. *Step 1* involves setting up the chamber for calibration. Make sure the chamber contains the pins or jaws, depending on the type of vessel being studied. If jaws are being used for smaller vessels, a wire needs to be strung on the transducer-side jaw for the calibration. Fill the chamber with double-distilled water for the volume to be used experimentally. Press "NEXT STEP".

CHAMBER 1 CALIBRATION [X]

Step no.: 1 2 3 4 5 6

Follow the Weight calibration procedure in the User Manual. Prepare the jaws and chamber for calibration. When ready go to next step.

[BACK] [NEXT STEP]

*Step 2* involves setting up the calibration kit appropriately for the actual weight calibration. Verify that the transducer arm pin does not touch the mounting wire on the jaw or the mounting pin for larger vessels, as instructed. The pin should be as close as possible to the mounting wire or mounting pin without touching in order to get the most accurate calibration. Press "NEXT STEP" when the calibration kit has been properly placed.


CHAMBER 1 CALIBRATION [X]

Step no.: 1 2 3 4 5 6


Place the calibration bridge on the myograph. Be careful when placing the bridge. The pin must not touch the wire/jaw. When ready go to next step.

[BACK] [NEXT STEP]


Step 3 initiates the heating process for the chambers. In order for the calibration to be accurate, the transducers must be heated to the experimental temperature to be used to accommodate heat-induced expansion of the electronic parts in the transducer. Otherwise, inaccurate readings and transducer drift may occur, introducing large errors into the experiment. To start heating, press “HEAT ON”.

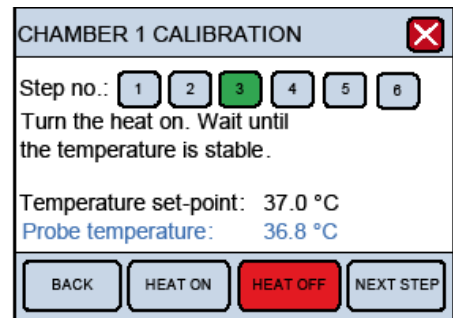


Covering the chambers with the chamber covers will expedite the chamber heating. Place the temperature probe into the chamber for the first calibration to monitor when the chamber has reached the target temperature. Heating will take about 20 to 30 minutes for the chambers and transducers to come to 37 °C with the chamber covers in place. Once the chamber(s) are heated and have reached the target temperature, press “NEXT STEP”.

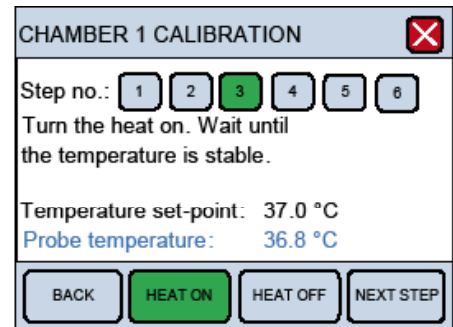


Step 4 is the first step in the actual weight calibration process. A 4-digit number will be displayed in blue at the bottom of the screen. If nothing has been perturbed during the heating process, the zero, 0 gram, or 0.00 mN calibration should be stable as indicated by the 4-digit number and “NEXT STEP” can be pressed at this time. If the 4-digit number is not stable, then wait until the number has stopped fluctuating before pressing “NEXT STEP”.

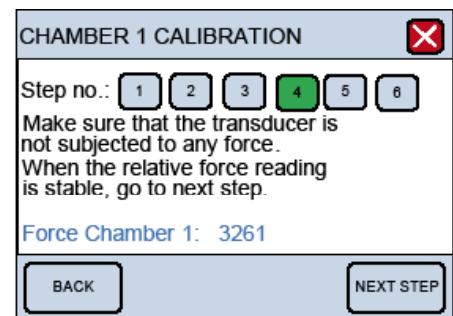

Step 5 is the 2 gram weight calibration. At this step, place the 2 gram weight in the pan closest to the transducer so as to simulate a vessel pulling on the jaw or pin attached to the transducer. Remember, a 2 gram weight in a 90° vector is cut in half, and the transducer will only detect 1 gram or 9.81 mN of force. The weight placement should cause a positive increase in the 4-digit number. Wait at least 10 to 15 seconds for the applied force to stabilize before pressing “NEXT STEP”. Once the 4-digit number has stabilized, press “NEXT STEP”.

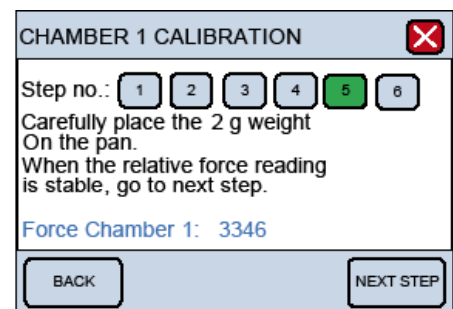


Step 6 is to verify that the calibration was performed correctly. The “Force Chamber 1” reading should be  $9.81 \pm 0.1$  mN. If the “Force Chamber 1” reading is off by more than 0.1 mN, then remove the weight, press “BACK” to return to Step 4, and repeat the calibration process. If the “Force Chamber 1” reading is satisfactory, then press “NEXT STEP”. Calibrate the other chambers in the same manner.

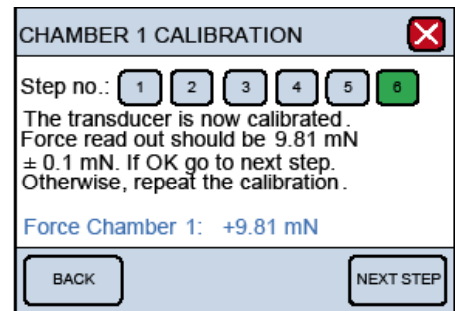


## 2. Valve delay:

Pressing “VALVE DELAY” in the SETTINGS menu will allow the user to modify the time duration that the vacuum valves stay open for washes. Factory default is set at 1 second, but 1 second is not enough time to completely empty a chamber with even as small a volume of 5 ml.

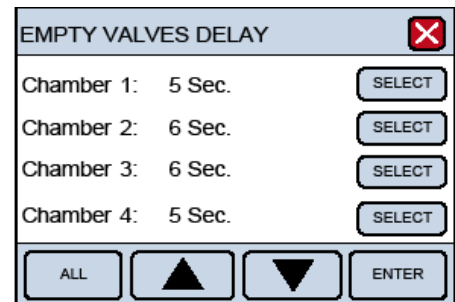


Pressing “SELECT” next to any given channel will cause the line selected to turn blue. The up and down arrow keys can then be used to modify the length of time the vacuum valves stay open after the valves have been activated with the push buttons on the front panel of the interface.

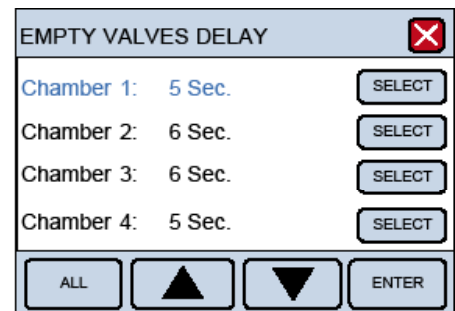

Pressing “ALL” will cause all the lines to turn blue, meaning all chambers can be modified at the same time. Again, the up and down arrow keys can be used to modify the length of time the vacuum valves stay open.

Pressing “ENTER” after modifying the value(s) for valve delay will lock in the number(s) and be retained in memory every time the system is turned on

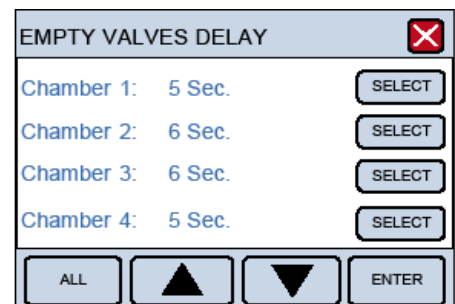

### 3. Force Rec. out:

The FORCE RECORDING OUTPUT, or FORCE REC. OUT, sub-menu determines the upper limit for force sent from the BNC analogue output connectors. This will only affect the data collected from the interface to a data acquisition system such as AD Instruments PowerLab and LabChart software. The factory default setting for FORCE REC. OUT is 20 mN, meaning that if the force of the mounted vessel exceeds 20 mN, the force recorded in the data acquisition software will not record more than 20 mN and will appear as a flat-line trace at 20 mN, even though the force readings on the interface may exceed 20 mN. Therefore, change the FORCE REC. OUT settings to an appropriate setting so as to capture any maximal response from the vessel of interest. This value should not exceed the settings for the transducer range, which is defined by the sub-menu, MEASUREMENT RANGE and is explained in the next section.

The “SELECT” and “ALL” functions are the same in this menu as previously described for the “VALVE DELAY” menu. Pressing “ENTER” will store the numbers in memory for future experiments.

Anytime this function is changed, a new weight calibration on the transducers should be performed, entering the new voltage values into the data acquisition system being used.

FORCE REC. OUTPUT RANGE			✕
Force1 Rec. Range.	200 mN	SELECT	
Force2 Rec. Range.	1100 mN	SELECT	
Force3 Rec. Range.	20 mN	SELECT	
Force4 Rec. Range.	1200 mN	SELECT	
ALL	▲	▼	ENTER

FORCE REC. OUTPUT RANGE			✕
Force1 Rec. Range.	200 mN	SELECT	
Force2 Rec. Range.	1100 mN	SELECT	
Force3 Rec. Range.	20 mN	SELECT	
Force4 Rec. Range.	1200 mN	SELECT	
ALL	▲	▼	ENTER

### 4. Measurement Range:

The MEASUREMENT RANGE sub-menu in SETTINGS determines the maximum force capacity of the transducer. The factory setting is 200 mN, but the transducer capacity can be changed to 400 mN, 800 mN or a maximum of 1600 mN of force detection, depending on the size of the vessel used.

The “SELECT” and “ALL” functions are the same in this menu as previously described for the “VALVE DELAY” menu. Pressing “ENTER” will store the numbers in memory for future experiments.


MEASUREMENT RANGE			✕
Range Chamber 1:	200 mN	SELECT	
Range Chamber 1:	800 mN	SELECT	
Range Chamber 1:	400 mN	SELECT	
Range Chamber 1:	200 mN	SELECT	
ALL	▲	▼	ENTER

MEASUREMENT RANGE			✕
Range Chamber 1:	200 mN	SELECT	
Range Chamber 1:	800 mN	SELECT	
Range Chamber 1:	400 mN	SELECT	
Range Chamber 1:	200 mN	SELECT	
ALL	▲	▼	ENTER

5. Interface settings:


The INTERFACE SETTINGS sub-menu in SETTINGS has an additional 2 sub-menus. These 2 additional sub-menus are:

- I. TEMPERATURE DIFFERENCE
- II. FACTORY DIAGNOSTICS

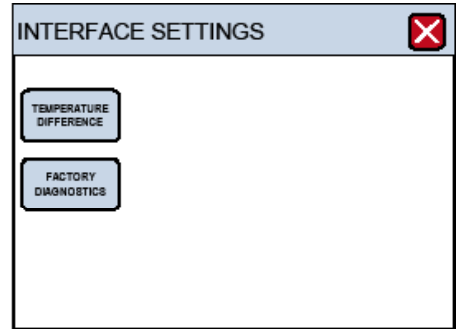


I. TEMPERATURE DIFFERENCE:

The TEMPERATURE DIFFERENCE function allows the user to finetune the temperature setpoint of the system. Although the temperature setpoint for the system can be set in the **HEAT MENU**, the actual temperature for the system may not heat to the exact defined setpoint. Therefore, the user can adjust the temperature of each chamber individually to fine-tune the temperature setting so that EXACT temperatures can be achieved for any particular chamber. This is referred to as a temperature offset (TEMP OFFSET ON CHAMBER).

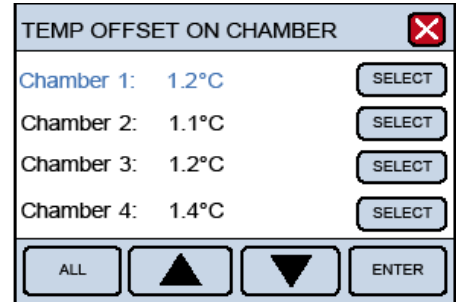


The “SELECT” and “ALL” functions are the same in this menu as previously described for the “VALVE DELAY” menu. Pressing “ENTER” will store the numbers in memory for future experiments.

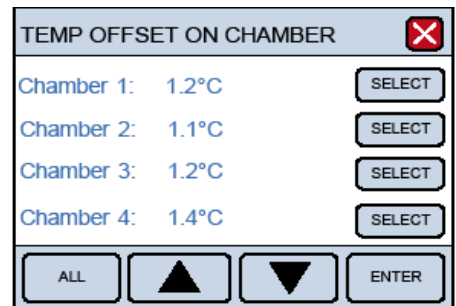

II. FACTORY DIAGNOSTICS:

Entering FACTORY DIAGNOSTICS will display the LOGIN CODE TO DIAGNOSTICS window. This window is for trained technicians and used for diagnostics and troubleshooting purposes. The general user will not have access to this window. Entering the proper 5-digit pin number, however, will allow the trained technician access to Diagnostics panels that will provide information during a malfunction or mechanisms to change other settings controlled by the onboard computer.

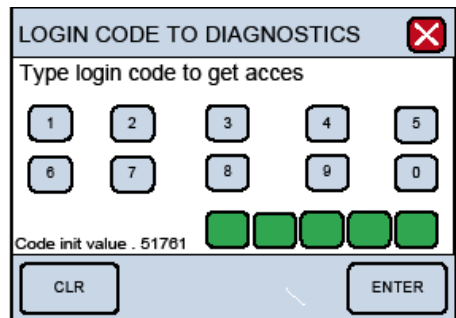

## CHAPTER 4 - THE MULTI WIRE MYOGRAPH UNIT

This chapter contains a complete explanation of how to adjust, calibrate and maintain the myograph 620M system so that the myograph is always performing at peak performance.

### 4.1 Changing and adjusting the mounting supports

Each chamber can accommodate mounting supports for either small vessels ( $>50\mu\text{m}$ ) or larger segments ( $>500\mu\text{m}$ ). Because the mounting supports can be changed easily, experiments can be performed with different vessels of varying internal diameter. Continuous use and repeated greasing of the transducer arm holes will cause some misalignment of the mounting supports. The mounting supports, therefore, whether they are the jaws for wires or the pins, will need occasional adjustments.

Changing and adjustment of the supports is performed using the following step-by-step procedure.

#### NOTE:

**THE TRANSDUCERS ARE FRAGILE AND SENSITIVE TO MECHANICAL STRAIN. BE VERY CAREFUL WHEN CHANGING OR ADJUSTING THE MOUNTING SUPPORTS!**

Changing the supports (Figure 4.1):

1. Use the micrometer to separate the supports as far apart as possible.
2. Use the small screwdriver provided to gently loosen screw D on the support attached on the transducer side using the small screwdriver. Screw D is the screw on the transducer-side support closest to the transducer.
3. Gently pull the support away from the transducer pin.
4. Loosen screw B on the micrometer side with the appropriate fitting allen key.
5. Pull the support away. Note: Number the supports with the chamber number they were removed from using some kind of permanent marker. Store the supports in the provided plastic case. Numbering the supports will save time when the supports are changed again, limiting the amount of adjustments needed after each change.

Course-adjusting the jaws for small vessels (Figure 4.1):

6. Loosen screw A to move the micrometer-side jaw toward or away from the micrometer.
7. Loosen screw D to move transducer-side jaw toward or away from the transducer.
8. Loosen screw C to vertically align the transducer-side jaw. Screw C is the screw on the transducer-side support that is furthest away from the transducer.

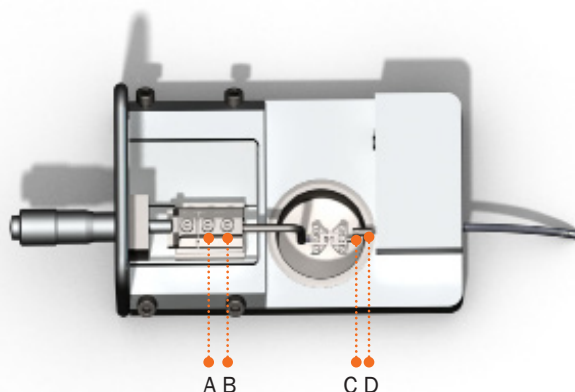


Figure 4.1 Myograph unit - screws for changing supports and coarse adjustment of the jaws

Fine-adjusting the jaws for small vessels (Figure 4.2 and Figure 4.3):

- 9. Tightening Screw I will move the micrometer-side jaw downward and to the left.
- 10. Tightening both screws I and III will move the micrometer-side jaw straight down.
- 11. Tightening both screws II and IV will move the micrometer-side jaw straight up.

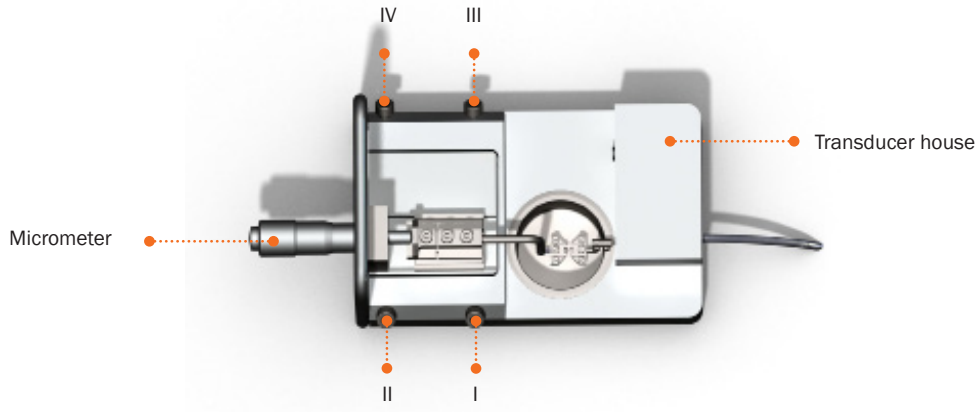


Figure 4.2 Fine adjustments of the jaws in the myograph chamber

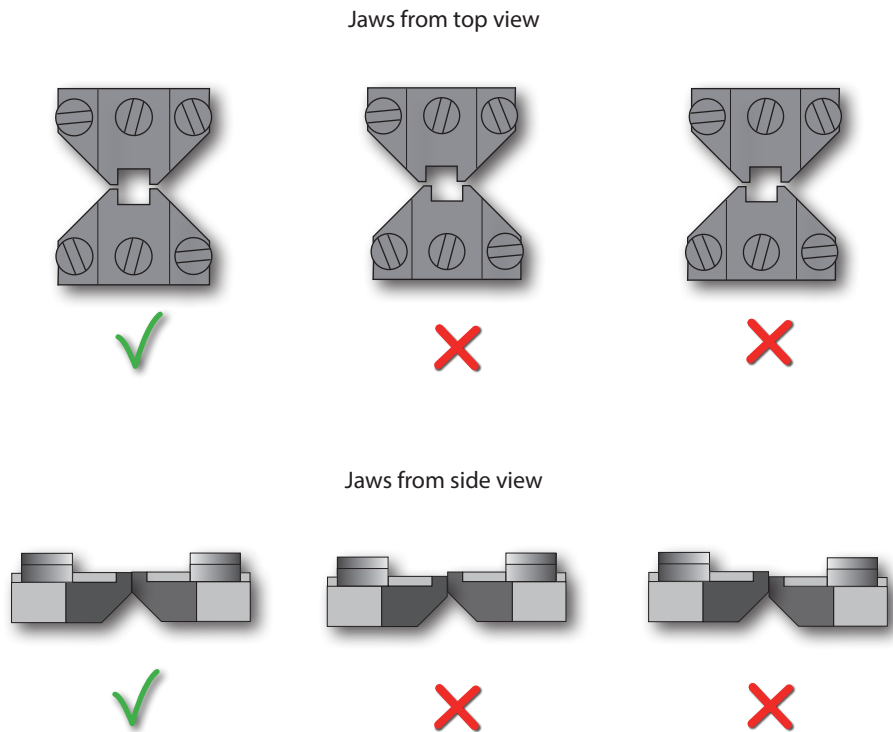


Figure 4.3 - Illustrations of properly aligned jaws (depicted on the far left) and incorrectly aligned jaws (depicted in the middle and far right).



Fine-adjusting the pins for larger vessels (Figure 4.4 and Figure 4.5):

12. Loosen screw A to move the micrometer-side arm holder sideways
13. Loosen screw B to move the micrometer-side pin toward or away from the transducer.
14. Loosen screw C to align the transducer-side pin horizontally.
15. Loosen screws D and E to align the heights of the pins vertically.

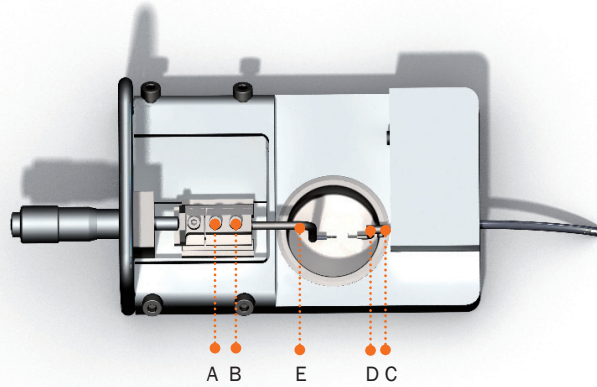


Figure 4.4 - Fine adjustments of the pins in the myograph chamber

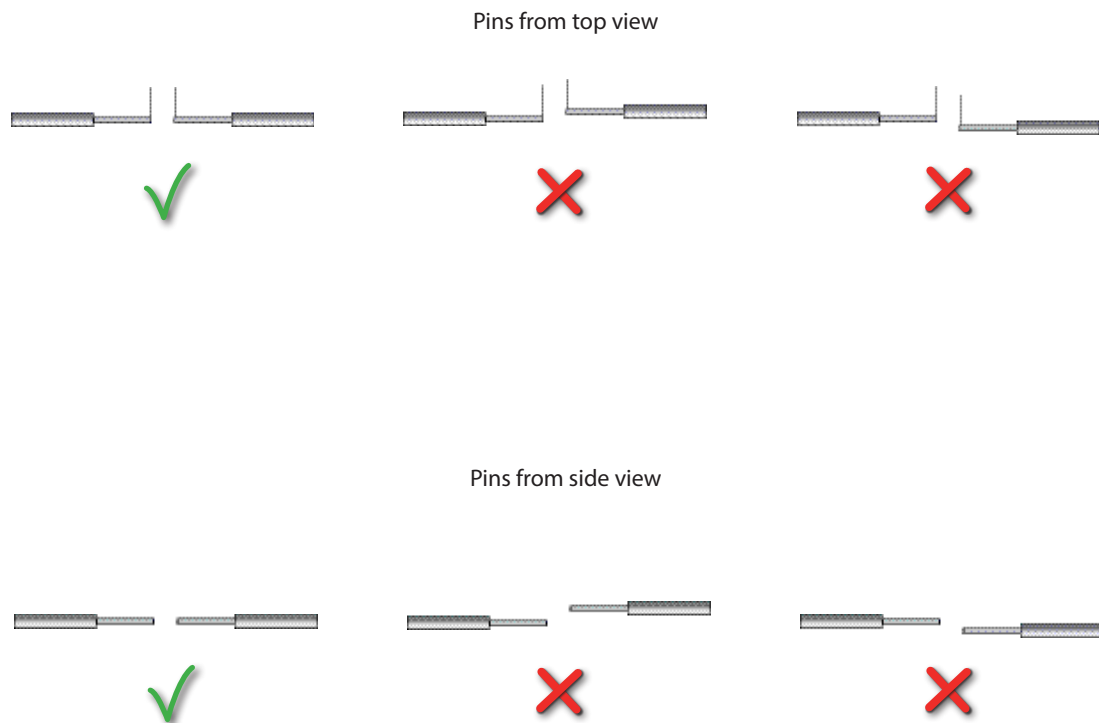


Figure 4.5 - Illustrations of properly aligned pins (depicted on the far left) and incorrectly aligned pins (depicted in the middle and far right).

## 4.2 Calibration of the force transducer

As a part of the general maintenance of the myograph, DMT recommends that the myograph is weight-calibrated at least once a month. The myograph should also be weight-calibrated every time the interface has been moved. Although lab benches are all supposedly perfectly horizontal, small differences in lab bench pitch can affect the calibration of the system. The myograph also should be calibrated if the system has been idle for longer than a month. A step-by-step procedure is included in the FORCE CALIBRATION sub-menu under SETTINGS, as explained in Chapter 3. See Appendix 3 for Principles of the Weight Calibration.

### Force transducer calibration procedure

This section contains step-by-step instructions to calibrate the force transducer and should be used in conjunction with the steps described in Chapter 3 (FORCE CALIBRATION sub-menu under SETTINGS).

**NOTE: EVERYTIME A FORCE CALIBRATION IS PERFORMED THE MEASUREMENT RANGE IS SET TO DEFAULT 200 mN. SET MEASUREMENT RANGE AFTER THE FORCE CALIBRATION.**

1. Move the jaws/pins apart. If calibrating the transducer with the jaws in place, make sure a wire is mounted on the transducer-side jaw. If pins are being used, the wire does not have to be put in place. Fill the chamber with distilled water or buffer. Use the same volume that will be used during the experiments.
2. Set up the calibration kit (bridge and balance) on one of the myograph chambers as illustrated in Figure 4.6. Also place the weight on one of the chambers. Turn the heat on as discussed in Chapter 3. The system takes about 20 to 30 minutes to reach 37 °C. Obviously, lower temperatures take less time and higher temperatures take more time to reach. Make sure adequate time is allowed so that calibration can be performed at the temperature at which the experiments will be performed. Placing the calibration kit and weight on the chamber allows them to warm up to the experimental target temperature. No need to bubble the chambers while waiting for the system to heat up.

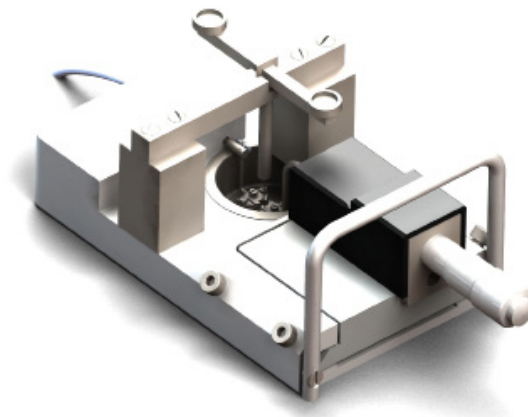


Figure 4.6 - Weight calibration kit shown in place on a single myograph chamber

3. When the system reaches target temperature, adjust the calibration kit so that the tip of the transducer arm is as close to the wire (if jaws are being used) or pin on the transducer side as possible without touching, as illustrated in Figure 4.9. One way to do this is to use the following technique. Start with the calibration kit in place so that the transducer arm of the bridge with the pans is not touching any part of the jaw or wire (if the jaws are being used) or not touching any part of the pins. Go to the main menu displaying the forces, and zero the channel being calibrated so the force reads zero. Slowly and gently slide the calibration kit forward toward the micrometer so that the transducer arm rests on the wire or pin, creating a force reading on that channel. Carefully slide the calibration kit back toward the transducer slowly until the force reads zero or very close to zero. At this point, as soon as the force reads zero, the transducer arm will be properly placed for weight calibration.
4. Go to the FORCE CALIBRATION sub-menu of the SETTINGS menu on the Interface to begin the actual transducer calibration. The process that is described above is reiterated in 6 steps once the FORCE CALIBRATION sub-menu is initiated, which is described in detail in Chapter 3.



Figure 4.7 - Illustration of the proper placement for the balance transducer arm for calibration

### 4.3 Checking the force transducer

The myograph force transducer is a strain gauge connected to a Wheatstone bridge. The force transducers for each chamber are housed in a separate, protective compartment (See Figure 4.8 below). While the protective cover offers some mechanical protection for the force transducers, they are still very vulnerable to applied forces exceeding 1 Newton (100 grams) or fluid running into the transducer compartment due to insufficient greasing of the transducer pinhole.

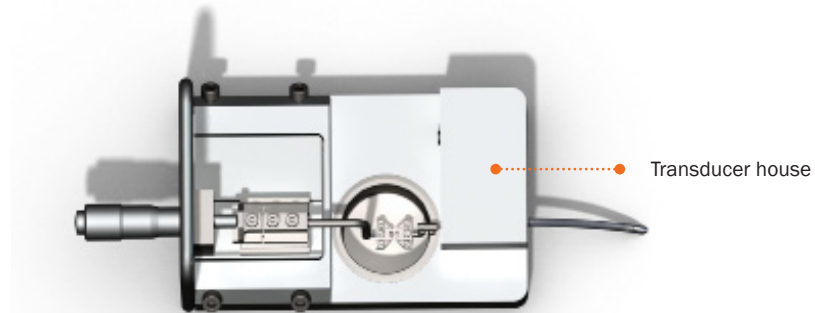


Figure 4.8 - Illustration of the proper transducer house

If the force readings on the Interface appear unstable or noisy, then first check that the chambers are connected properly to the Interface and that the chambers are plugged all the way into the interface.

If the force reading(s) are still unstable or noisy, then perform a new calibration of the force transducer as described in Chapter 3 and Chapter 4.2.

During the new calibration, monitor the relative force reading values in the FORCE CALIBRATION sub-menu on the Interface (Steps 4 and 5 of the calibration procedure). The normal operating values for the force transducer during calibration should be between 3000 and 3500.

- If the value is 0, a single digit, or a three digit number, the force transducer is broken and needs to be replaced.
- If the value is less than 2000 or greater than 4500, the force transducer is broken and needs to be replaced.
- If the message "OFF" is displayed on the main page of the Interface, even though the chamber is plugged in at the rear of the interface, the force transducer is broken and needs to be replaced. In addition, if the force reading(s) appear yellow in color, cannot be reset to zero, AND the transducer cannot be recalibrated, the force transducer is broken and needs to be replaced.

If any other problems related to the force transducer are encountered, please contact DMT for advice or further instructions.

## 4.4 Force Transducer Replacement

If the force transducer breaks and needs to be replaced, follow this step-by-step replacement procedure carefully:

1. Remove the pin or jaw from the transducer pin coming out of the transducer house.
2. Disconnect the Myograph Chamber from the Interface.
3. Turn the Myograph Chamber upside down and remove the transducer housing by loosening the two screws (A+B) as illustrated in Figure 4.9 below.



Figure 4.9 - The 2 screws that secure the transducer house to the chamber

4. The replacement transducer will be shipped with the new transducer inside a new transducer house.
5. Place a small amount of vacuum grease (clear or whitish grease) around the bottom of the transducer housing to seal the transducer housing when put back in place.
6. Carefully realign the transducer housing with the new transducer on the Myograph Chamber and reinsert the allen screws through the bottom of the Myograph Chamber.
7. Tighten the screws and place some vacuum grease around the transducer pin that protrudes from the transducer housing. Make sure that the hole is completely sealed to prevent buffer solution or water from entering the transducer housing and damaging the new force transducer.

### IMPORTANT NOTE:

CALIBRATE THE NEW FORCE TRANSDUCER BEFORE PERFORMING A NEW EXPERIMENT, AS DESCRIBED IN CHAPTER 3 AND 4.2.

## 4.5 Myograph Maintenance

The Multi Wire Myograph System Model 620M is a very delicate and sophisticated piece of research equipment. DMT recommends that the following sections are read carefully and that the instructions are followed at all times.

### Myograph chamber tubing

To prevent the tubing from becoming blocked with buffer salt deposits after an experiment, remove the chamber cover from the Myograph Chamber and turn on the vacuum and press the vacuum valve for about 10 seconds by holding down the valve button(s) down. Turn off the vacuum and gas supply. Remove any water or buffer remaining in the chamber or on the tubing using absorbent paper.

### Force transducer

The force transducer is the most delicate and fragile component of the myograph system. Extreme care must be used when handling or touching the force transducers.

As a part of daily maintenance, inspect the grease around the transducer pin extending from the transducer housing pinhole before starting any experiment. Insufficient grease in this area will allow buffer and water to enter the transducer housing and cause damage to the force transducer.

### IMPORTANT NOTES:

- DMT RECOMMENDS THAT THE HIGH VACUUM GREASE SEALING THE TRANSDUCER PINHOLE IS CHECKED AND SEALED AT LEAST ONCE A WEEK, ESPECIALLY IF THE MYOGRAPH IS USED FREQUENTLY.
- DMT TAKES NO RESPONSIBILITIES FOR THE USE OF ANY OTHER KINDS OF HIGH VACUUM GREASE OTHER THAN THE ONE AVAILABLE FROM DMT.
- DMT TAKES NO RESPONSIBILITIES FOR ANY KIND OF DAMAGE APPLIED TO THE FORCE TRANSDUCERS.

### Linear slides

Check the linear slides (under the black covers) for grease at least once a week. In case of insufficient lubrication, grease the slides with the "Grease for Linear Slides" included with your system.

### Cleaning the myograph

DMT strongly recommends that the myograph chambers and surrounding areas are cleaned after each experiment.

At the end of each experiment, use the following procedure to clean the myograph chambers and supports:

1. Fill the myograph chamber to the edge with an 8% acetic acid solution and allow it to work for a few minutes to dissolve calcium deposits and other salt build-up. Use a cotton-tipped applicator to mechanically clean all chamber surfaces.
2. Remove the acetic acid and wash the myograph chamber and supports several times with double distilled water.
3. If any kind of hydrophobic reagents have been used which might be difficult to remove using steps 1) and 2), then try incubating the chamber and supports with 96% ethanol or a weak detergent solution (i.e. 0.1% triton-100).
4. To remove more resistant or toxic chemicals, incubate the myograph chamber and supports with 1M HCl for up to 1 hour. In exceptional cases, incubate the chamber and supports with no stronger than a 3M HNO<sub>3</sub> solution for about 15 minutes.
5. Wash the myograph chamber and supports several times with double distilled water.
6. If acids such as 1M HCl and 3M HNO<sub>3</sub> are used to clean the chambers, make sure ALL surfaces are thoroughly dried after copious washes with double distilled water. Any residual acid will cause corrosion of the stainless steel jaws and pins.

### IMPORTANT NOTES:

- BE VERY CAREFUL USING HCL OR HNO<sub>3</sub> BECAUSE THESE ACIDS MAY CAUSE EXTREME DAMAGE TO THE STAINLESS STEEL CHAMBERS AND SUPPORTS. DO NOT USE BLEACH TO CLEAN THE CHAMBERS. REPEATED USE OF CHLORINATED SOLUTIONS SUCH AS BLEACH AND HCL WILL CAUSE DAMAGE TO THE STAINLESS STEEL PARTS OF YOUR MYOGRAPH SYSTEM. AVOID USING THEM IF AT ALL POSSIBLE.
- AFTER CLEANING, ALWAYS CHECK THAT THE GREASE AROUND THE TRANSDUCER PIN IS SUFFICIENT TO KEEP THE BUFFER AND WATER FROM ENTERING THE TRANSDUCER HOUSING.

If red or brown discolorations appear on the chamber sides or on the supports, the following cleaning procedure will work in most cases:

7. Incubate the myograph chamber and supports for 30 minutes with 2mM T-1210 Tetrakis- (2-pyridylmethyl)-ethylenediamine solution dissolved in double distilled water.
8. Use a cotton-tip applicator to mechanically clean all the affected surfaces during the last 15 minutes of the incubation period.
9. Wash the myograph chamber and supports several times with double distilled water.
10. Incubate the myograph chamber with 96% ethanol for 10 minutes while continuing the mechanical cleaning with a cotton-tip applicator.
11. Remove the ethanol solution and wash a few times with double distilled water. Incubate the myograph chamber and supports with an 8% acetic acid solution for 10 minutes and continue the mechanical cleaning with a swab-stick.
12. Wash the myograph chamber and supports several times with double distilled water.
13. Dry the surfaces using absorbent paper (i.e. Kim-Wipes) or cotton-tip applicators.

#### IMPORTANT NOTES:

IN EXCEPTIONAL CASES, THE SUPPORTS (JAWS OR PINS) MAY NEED TO BE REMOVED FROM THE MYOGRAPH CHAMBER AND CLEANED INDIVIDUALLY TO ASSURE PROPER CLEANING OF ALL SUPPORT SURFACES. NEVER SOAK THE SUPPORTS IN ANYTHING STRONGER THAN 8% ACETIC ACID FOR EXTENDED PERIODS OF TIME (I.E. SEVERAL HOURS OR OVERNIGHT)!

# APPENDIX 1 - SYSTEM SPECIFICATIONS

## Technical specifications

Vessel size:	>60 µm / >450 µm up to 10 mm
Chamber:	Four individual chambers
Chamber material:	Acid-resistant stainless steel
Chamber volume:	Max. 8 ml
Chamber suction:	Manual or automatic, time controlled, user defined
Chamber cover:	Supplied with connections for gassing
Chamber gassing:	Individually controlled per chamber by needle valves
Force range:	User selectable at ± 200/400/800/1600 mN
Force resolution:	0.1 mN
Micropositioners:	Manually operated precision micrometer
Weight calibration:	Semi Automatic
Heating:	Built into chamber, independent of superfusion
Temp. range:	Ambient temp. - 45 °C
Temp. resolution:	0.1 °C
Temp. probe:	External
Output reading:	Force (mN)
Analogue output:	Independently filtered 4-channel output at 2.5V full scale
Voltage:	100 to 240 VAC (auto) 50/60 Hz via external power supply
Ambient temp.:	15-30 °C

## Optional accessories

Automatic Buffer Filler System - 625FS  
Chamber cover for field stimulation  
Plastic mounting jaws for field stimulation  
Combined pulse & train generator - CS200



# NOTES